

User Manual

User manual no.:

IMMU-12-03-04-14-ENG

MOISTURE ANALYZER MAC SERIES



BALANCES AND SCALES

RADWAG 26 – 600 Radom, Bracka 28, POLAND

Phone: +48 (0-48) 38 48 800, fax. +48 (0-48) 385 00 10

export@radwag.com

www.radwag.com

MARCH 2014


1.	TECHNICAL DATA	5
2.	GENERAL SAFETY INFORMATION	6
2.1.	Definitions of signals and warning signs	6
2.1.1.	Warning descriptions	6
2.1.2.	Warning signs	6
2.2.	Safety information	7
2.3.	Intended use	9
2.4.	Inappropriate use	10
2.5.	Principles of safety use	10
2.6.	Warranty	11
2.7.	Monitoring metrological parameters of the instrument	11
2.8.	Data included in this user manual	11
2.9.	Staff competence	11
2.9.1.	Protective clothing	12
3.	TRANSPORT STORAGE	12
3.1.	Delivery check	12
3.2.	Packaging	12
4.	UNPACKING, ASSEMBLING AND STARTUP	12
4.1.	Assembling and place of use	12
4.2.	Unpacking	13
4.3.	Level setting	14
4.4.	Standard delivery components	14
4.5.	Cleaning	14
4.6.	Plugging to mains	15
4.7.	Connecting peripheral equipment	15
5.	KEYBOARD – FUNCTION KEYS	16
6.	START-UP	17
6.1.	Moisture analyzer temperature stabilization period	17
7.	USER MENU	18
7.1.	Moving through user menu	18
7.2.	Return to weighing mode	21
8.	WEIGHING	22
9.	MOISTURE ANALYZER MAIN PARAMETERS. ADJUSTING MOISTURE ANALYZER OPERATION TO AMBIENT CONDITIONS AT A WORKSTATION	22
9.1.	Setting filtering level	23
9.2.	Autozero function	24
9.3.	Access to library of drying programs	25
9.4.	Backlight of measurement result (display backlight)	26
9.5.	Brightness adjustment of display backlight	27
9.6.	“beep” sound – reaction on pressing a function key	27
10.	MOISTURE ANALYZER ADJUSTMENT	28
10.1.	External adjustment	29
10.2.	Adjustment test	30
10.3.	Drying chamber adjustment	31
10.4.	Adjustment report printout	34
10.5.	Drying process test	35

11.	DETERMINING CONTENT OF A PRINTOUT FOR GLP PROCEDURES	37
12.	DATE AND TIME SETTINGS	40
12.1.	Setting time	40
12.2.	Setting date	41
13.	RS 232 FUNCTIONS	41
13.1.	Baud rate setting	41
13.2.	Determining data type sent via RS 232 output	42
13.3.	Printout interval	43
13.4.	Determining range of data sent during drying process	43
14.	DRYING PROCESS WITH USE OF SHORTENED MENU	44
14.1.	Setting means of auto switch off mode	45
14.2.	Active drying mode	46
14.3.	Type of displayed measurement result	49
15.	DRYING PROCESS WITH USE OF DRYING PROGRAM LIBRARY	50
15.1.	Sample mass control	51
16.	DRYING PROCESS	52
17.	SET OF COMPUTER – MOISTURE ANALYZER COMMANDS	56
18.	ERROR MESSAGES	58
19.	PRINCIPLES OF USE	58

1. TECHNICAL DATA

Type	MAC 50/1	MAC 50	MAC 110	MAC 210
Max capacity	50 g	50 g	110 g	210 g
Readability	0,1 mg	1 mg	1 mg	1 mg
Tare range	- 50 g	- 50 g	- 110 g	- 210 g
Max sample mass	50 g	50 g	110 g	210 g
Readability of moisture readout	0,0001%	0,001 %		
Repeatability of moisture content reading	+/-0,1% (sample ~ 2g), +/-0,02% (sample ~10g)			
Drying temperature range	max. 160 °C max. 250 °C (WH)			
Heating module	halogen (WH) infrared emitter heater in metal cover (NS)			
Drying modes	4 drying modes: standard, quick, step, mild			
Auto switch off option	3 modes: automatic, time defined, manual			
Working temperature	+10 °C - +40 °C			
Power supply	230V 50Hz AC / 400W			
Display	LCD (backlit)			
Pan size	Φ 90 mm, h = 8 mm			
Drying chamber dimensions	120 x 120 x 20 mm			
Net weight / Gross weight	4,9 / 6,4 kg			
Packaging dimensions	470 x 380 x 336 mm			

Dimensions:

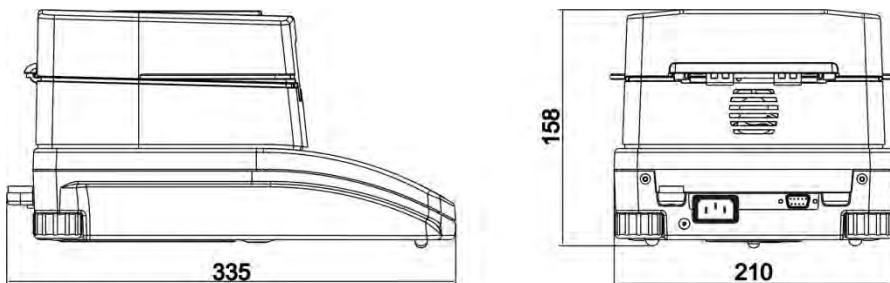

2. GENERAL SAFETY INFORMATION

2.1. Definitions of signals and warning signs

Safety precautions are marked with special descriptions and warning signs. They inform and warn a user of possible dangers. Ignoring the safety warnings may cause injuries, damage of the moisture analyzer, its inappropriate operation and errors of measurements.

2.1.1. Warning descriptions

WARNING

Dangerous situations of high risk. These situations can cause serious injuries or death if the safety precautions are not taken.

CAUTION

Dangerous situations of low risk. These situations can cause damage of the instrument or its functions, loss of data as well as minor or moderate body injuries.

ATTENTION

Important information related to the moisture analyser.

2.1.2. Warning signs



Electric shock risk



Acid / Corrosion



Danger



Flammable or explosive substances



Toxic substances



Hot surfaces

2.2. Safety information

CAUTION!

The use of moisture analyzer MA 3Y regardless of both, safety information and user manual guidelines may cause health damage and even death



WARNING:

Nominal voltage for a moisture analyzer is 230 VAC. It means that safety usage precautions for low voltage devices must be abide by while operating the device.

Three-core power supply cable with grounding pin comes standard with a moisture analyzer.

If necessary, an extension cord can be used as long as it meets

the applicable standards and has a protective ground conductor. Intended disconnection of the grounding cable is

forbidden.



CAUTION:

Drying chamber cannot be opened during operation (drying process). It is due to the fact that a halogen lamp and its glass shield may reach the temperature of up to 400 C.

When setting up the moisture analyzer leave enough space to

prevent heat from building up and to keep your analyzer from

overheating. Leave about 20 cm around the instrument and about 1 m above.

Air vents that are located in the housing cannot be covered, sealed or blocked in any other way.

Do not put any flammable substances on, under or near the moisture analyzer.

Be particularly careful when removing the sample from the drying chamber: the sample itself, the drying chamber, shields

and the pan can still be extremely hot.

In case of any maintenance work (cleaning the inside of the drying chamber), the moisture analyzer must be switched off.

Wait until all the components have cooled down. Do not perform

any modification to the heating module.

Same types of samples require taking particular safety precautions.

They can pose a danger for people and objects. It is always the user who is liable for possible damages caused by the use of an inappropriate sample.



CAUTION:

Corrosion

Substances that release aggressive vapours (e.g. acids) during

the heating process. In this case, it is recommended to work with

small samples. Otherwise, vapours can condense on cold housing parts and cause corrosion.



WARNING:

Fire or explosion

Flammable or explosive substances, substances containing solvents or releasing flammable or explosive gases or vapours.

Perform a risk analysis when in doubt relating to the sample characteristics before carrying out the procedure.

For this type of samples apply the drying temperatures as low as possible to prevent flames or explosion. During the analysis it is

necessary to wear protective glasses and gloves. The samples

should be relatively small.

Under no circumstances can the instrument be left Unsupervised!



WARNING:

Substances containing toxic and caustic or corrosive components

Substances that release toxic gases or vapours can cause irritations (eyes, skin or respiratory system), illnesses or even death. Dry such substances only in fume hood.

Under no circumstances should the instrument be used in an area with any risk of explosion. The moisture analyzer is not designed to operate in hazardous areas.

2.3. Intended use

A moisture analyzer MA 3Y series is designed to determine relative moisture content in small samples of various substances, determine dry mass content in small samples and determine mass of weighed objects.

MA 3Y ensures fast and precise determination process of water content in a tested sample, and application of touch screen display considerably simplifies operation and improves functionality of the moisture analyzer. A moisture analyzer MA 3Y series can be used to determine humidity content of different materials.

At the initial stage of measurement, the device precisely determines the mass of an object placed on instrument's weighing pan. As the mass reading is stabilized, the sample is quickly heated by a halogen lamp, an IR emitter or a metal heater causing humidity evaporation from the tested sample. While sampling, the moisture analyzer is continuously checking the loss of mass, and on calculation, it displays current moisture content in a tested sample. Compared to conventional methods of humidity content determination of various substances, application of moisture analyzer MA 3Y series


considerably shortens measurement time and simplifies testing procedure. MA 3Y series allows for setting multiple parameters which influence the procedure of moisture content determination in a sample, such as: temperature, time, drying modes, etc.

2.4. Inappropriate use

CAUTION!

Do not open the drying chamber during drying process. Moisture analyzer features a halogen lamp which is a very powerful heat source. Thus, user should pay special attention not to touch those elements of a moisture analyzer that get hot while drying procedure (i.e.: disposable pan, pan handle, and inner shields of the drying chamber).

Remember that some of tested samples may become dangerous if heated (appearance of poisoning vapours, danger of ignition or explosion).

Moisture analyzer MA 3Y series is not intended for dynamic weighing. Even if small amounts of a sample are added to taken off the weighing pan, the mass readout should only be taken only on stabilization of measurement result (appearance of stability pictogram  on the display).

Do not place any magnetic materials on the weighing pan, as this can cause damage of the measuring system of the instrument. Be sure to avoid impact shock and overloading the moisture analyzer in excess of the prescribed maximum measuring range (max capacity), minus any possible tare weight that has been applied).

Never use the moisture analyzer in an environment endangered by an explosion!

This moisture analyzer is not adjusted for operation in explosive areas. There must not be any modification made to the moisture analyzer.

2.5. Principles of safety use

Moisture analyzer is in accord with all binding safety regulations. Nevertheless there are exceptional circumstances that may cause danger.

It is forbidden to open an instrument housing. Inside there are no parts that would require maintenance, repair or replacement carried out by a user. In case of any problems it is recommended to contact RADWAG service or a distributor. It must be always remembered to use the device in accordance with this service manual and especially to follow instructions on installation and configuration of a new device.

Use of a moisture analyzer MA 3Y series conversely to safety principles and user manual guidelines may be hazardous to operator's health and life. It is obligatory to acknowledge the safety principles listed in the user manual:

- use a moisture analyzer only to determine humidity content in samples and determine mass of a tested sample. Any other use of the moisture analyzer may be dangerous both to the device and the user,
- before commissioning the moisture analyzer, make sure that the nominal power of the device specified on its data plate, is compatible

with the supply in the mains to which the moisture analyzer will be plugged in,

- **replecment of halogen lamps can only be carried out by authorized service,**
- protect moisture analyzer against contacts with liquids, it might lead to electrocution, fire, emission of substances containing toxic or caustic vapour, emission of explosive substances.

2.6. Warranty

Warranty does not cover the following cases:

- Not observing the regulation listed in user manual,
- Using the moisture analyzer conversely to its intended use,
- Any modifications of moisture analyzer or cases when its housing is opened (damaged protective stickers),
- Mechanical defects and defects caused by media, liquids, water and natural wearing off,
- Improper placing of defects of electrical network / mains,
- Overloading of measuring mechanism of the moisture analyzer.

2.7. Monitoring metrological parameters of the instrument

Metrological characteristics of the moisture analyzer requires periodical inspection carried out by its operator. Inspection frequency is conditioned by ambient conditions in which the moisture analyzer is used, types of performed processes and accepted quality management system in an organization.

2.8. Data included in this user manual

Please read the user manual carefully before instrument's plugging to mains and startup, even if the user is experienced with this type of moisture analyzers.

2.9. Staff competence

Moisture analyzer MA 3Y series should only be operated and maintained by personnel who is trained and experienced in using this type of instruments.

In order to use the moisture analyzer, first read the user manual. Keep these instructions for the future reference.

Do not make any structural modifications. Additional equipment, which can be connected to the moisture analyzer, should be supplied by RADWAG or an authorized distributor.

2.9.1. Protective clothing

The use of protective clothing is highly recommended while working with the instrument in order to take safety precautions against potential hazards resulting from tested samples and ingredients.

Use the following while carrying out tests:

- protective apron,
- protective glasses,
- protective gloves (while working with hazardous chemical substances).

Before the use of the above-mentioned protective clothing, make sure that they are designed to be used with specific samples and they are not damaged.

3. TRANSPORT I STORAGE

3.1. Delivery check

Please check the packaging immediately upon delivery and the device during unpacking for any visible signs of external damage.

3.2. Packaging

Please retain all parts of the original packaging should the moisture analyzer be transported in the future. Only the original packaging should be used for dispatching the moisture analyzer. Before packing, disconnect all attached cables and remove any loose/movable parts (weighing pan, shields, inserts). Place moisture analyzer and its components in their original packaging, and protect them against damage during transport.

4. UNPACKING, ASSEMBLING AND STARTUP

4.1. Assembling and place of use

- A moisture analyzer should be stored and used in locations free of vibrations and shakes, free of air movement and dust, located at the max altitude of 2000 above sea level,
- Moisture analyzer's place of use should ensure good air circulation around the instrument (approximately 20 cm free space around the moisture analyzer and 1 m free space over it),
- Ambient air temperature in the weighing room should not exceed the range of:
 $+10^{\circ}\text{C} \div +40^{\circ}\text{C}$,


- Ambient relative humidity should not exceed 80% in the temperature up to 31 °C, and decrease linearly to 50 % of relative humidity in temperature 40 °C,
- A moisture analyzer should be located on a stable wall console desk or a stable working table which is not affected by vibrations and distant from heat sources,
- Take special safety measures when weighing magnetic objects, as part of the balance is a strong magnet.

4.2. Unpacking

Carefully remove the moisture analyzer from its packaging, remove the plastic and foil transport protective elements. Gently place the moisture analyzer in its intended place of use.


Assembly the components of drying chamber, following guidelines from below figure:

Assembling moisture analyzer components:

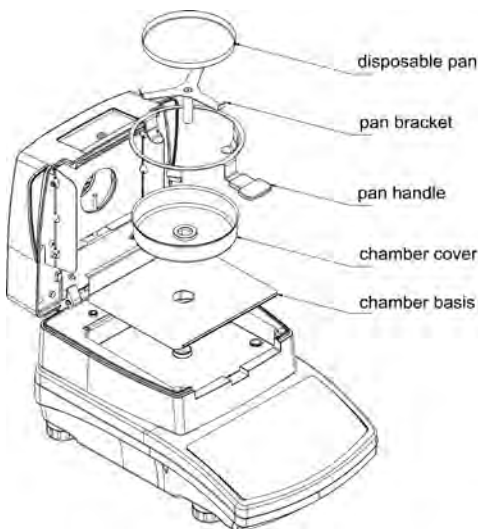

- Assembly insert of the drying chamber's basis
- Assembly drying chamber cover,
- Assembly drying pan handle,
- Assembly drying pan bracket,
- Assembly the disposable drying pan.

Setting drying pan's supporter (bracket).

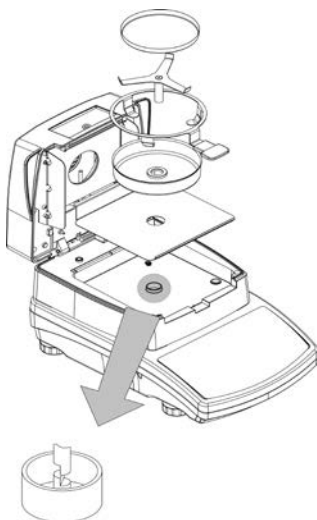

When assembling the pan supporter (bracket) pay special attention to the correct positioning of its mandrel. The mandrel features a cut for its unique positioning against the pan handle, thus preventing their contact and friction.

Setting pan's bracket:

- On assembling the pan bracket onto the mandrel, turn the bracket slightly, so that the cut on the mandrels are located in their unique and correct position,
- When turning the mandrel use most gentle movements not to damage moisture analyzer's measuring system.

4.3. Level setting



Before plugging to mains, level the moisture analyzer using adjustable feet. Turn the feet in a way that the air bubble of the level is located centrally.

4.4. Standard delivery components

- A moisture analyzer MAC series
- Insert of drying chamber basis.
- Drying chamber shield.
- Drying pan handle.
- Drying pan bracket.
- Disposable pan.
- Power cord.
- User manual (CD).

4.5. Cleaning

Remember to unplug the moisture analyzer from mains before any cleaning activities.

Clean the moisture analyzer using a damp cloth by gentle rubbing contaminated places. **Remember to remove the drying pan from the drying chamber before its cleaning. If the drying pan assembly is installed while being cleaned it may damage instrument's measuring system, thus remove it from the bracket.**

4.6. Plugging to mains

A moisture analyzer can be plugged to mains only by means of original power cord, which comes standard with the moisture analyzer. Rated voltage (specified on device's data plate) must be compatible with mains rated voltage.


The power cord can be connected only to socket with ground contact. Plug the power cord to the moisture analyzer. The moisture analyzer's power plug is located at the back of instrument's housing.

On plugging to mains moisture analyzer's displays software's name and number, after which the indication changes to 0.000 g (in case of a moisture analyzer with measuring accuracy 1 mg) or 0.0000 g (in case of a moisture analyzer with measuring accuracy 0,1 mg). In mass indication is other than zero press O/T key located on the overlay.

4.7. Connecting peripheral equipment

The moisture analyzer must be unplugged from the mains before connecting or disconnecting any peripheral equipment (printer, PC computer). Use only peripheral equipment recommended by the manufacturer with your moisture analyzer. These have been ideally coordinated to your moisture analyzer. On connecting a peripheral device, plug the moisture analyzer to mains.


5. KEYBOARD – FUNCTION KEYS

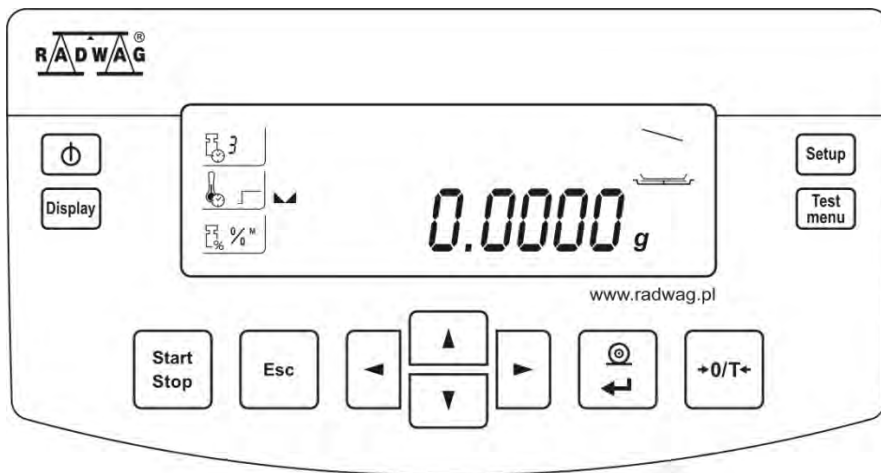

Start/Stop key – starting / ending drying process according to selected drying mode.



Esc key, abandoning introduced changes / exit one level higher in menu structure.



Group of navigation keys – change of parameters value; moving in moisture analyzer's menu.



Print/Enter key – sending display status to peripheral device (Print) or confirmation of selected value or function (Enter).



ZERO/TARE key – zeroing moisture analyzer's indication.



On/Off key – switch on/off display of moisture analyzer. On switching of the display of the device, other subassemblies are continuously supplied, and the moisture analyzer is in standby mode.



Display key – changes type of data displayed during and after drying process.



Setup key – enter to main menu.



Test menu key – function key for selecting drying modes.

6. START-UP

On plugging to mains the moisture analyzer carries out a display test (all pictograms and digits appear on the display). Then the display shows software name and number, and enters weighing mode.

6.1. Moisture analyzer temperature stabilization period

Before start of measuring processes, it is necessary to wait until the moisture analyzer is thermally stabilized. It is a period of so called moisture analyzer's self-heating.

For moisture analyzer MAC series which before plugging to mains was stored in room temperature, self-heating period takes approximately 30 minutes. For moisture analyzers that were stored in much lower temperatures before plugging to mains (e.g. during winter period) thermal stabilization should last approximately 4 hours.

During self-heating period the indications on moisture analyzer's display may change. Correct operation of a moisture analyzer is possible within temperature range specified in the technical parameters, see point 1.








It is recommended that ambient temperature changes at moisture analyzer's place of use are very small (slow).

7. USER MENU

User menu is divided into 5 basic function groups.

7.1. Moving through user menu

An operator moves through moisture analyzer's menu using keys on overlay's keyboard:

	Setup key. Entering main menu.
	Navigating key UP – Selecting group of parameters one by one upwards / changing parameter value by one value upwards.
	Navigating key DOWN – Selecting group of parameters one by one downwards / changing parameter value by one value downwards.
	Navigating key RIGHT – Selecting group of parameters for activating. On pressing the key, the display indicates the first parameter in a selected group.
	Navigating key LEFT – Exit to previous menu level, e.g. to main menu.
	Esc key. Abandon parameter changes.
	Print/Enter key. Accept / confirm introduced changes

Names of function groups and their content:

P1 CAL [Adjustment]

P1-01 ECAL		[external adjustment]
P1-02 tCAL		[adjustment test]
P1-03 tE_CAL		[drying chamber adjustment]
P1-04 CALr		[adjustment report printout]
P1-05 tSt_Co		[drying process test]

P2 GLP [Good Laboratory Practice]

P2-01 USr		—	[name of user]
P2-02 PrJ		—	[name of project]
P2-03 Ptin		YES/no	[printout of measurement time]
P2-04 PdAt		YES/no	[printout of measurement date]
P2-05 PUSr		YES/no	[printout of user name]
P2-06 PPrJ		YES/no	[printout of project name]
P2-07 PId		YES/no	[printout of moisture analyzer's factory no.]
P2-08 PFr		YES/no	[printout of frames]

P3 tinnE [Setting time and date of the moisture analyzer]

P3-01 StinnE		[setting time]
P3-02 SdAtE		[setting date]

P4 rEAd [Main user parameters]

P4-01 AuE		Stand/SLouu/Fast	[filtering level]
P4-02 Auto		On/OFF	[autozero]

P5 Print [Data transmission – RS 232]

P5-01 bAud		2400/4800/9600/19200	[baud rate]
P5-02 PStb		YES/no	[measurement result printout: stable / unstable]
P5-03 LinE_t		1/2/3/5/10/20/30/60/120/180	[printout interval]
P5-04 Prn_Pc		YES/no	[printout to computer]

P6 othEr [Other functions]

P6-01 Libr		YES/no	[access to drying modes library]
P6-02 bL		YES/no	[display backlight]
P6-03 bLbA		no/20/30/40/50/60/70/80/90/100	[display brightness]
P6-04 bEEP		YES/no	[beep sound on pressing keys]
P6-05 PrnS			[printout of moisture analyzer parameters]
P6-06 Preuer		YES/no	[prior moisture analyzer mode]

7.2. Return to weighing mode

CAUTION





Changes introduced in moisture analyzer memory will be permanently saved on return weighing with procedure of saving changes.

Press **Esc** key for several times, until the display indicates command **SAuE ?**



Then select one of below option:

- **Print/Enter**  - key – save (accept) changes
- **Esc**  - key – abandon introduced changes, and leave to balance menu.

8. WEIGHING

Before start of measuring process or in case of essential change of ambient conditions at a workstation (e.g. ambient temperature change at a workstation) the moisture analyzer requires adjusting. The procedure of moisture analyzer adjustment is described further in this user manual.

- Before start of measuring procedure, it is recommended to load the moisture analyzer's pan a few times with mass close to the max capacity,
- Check if unloaded moisture analyzer indicates "precise zero" - **→0←** and whether measurement is stable - **▲▲**, if not press **ESC/TARE** key,
- Place weighed object on moisture analyzer's weighing pan and read result only on stabilization of measurement result,
- Mass indication of a load placed on moisture analyzer's weighing pan can be tarred for multiple times by pressing **ESC/TARE** key (pay attention not to exceed maximal capacity of a moisture analyzer by applying multiple tare function).




During times between carrying out the following measurement series do not unplug the moisture analyzer from mains. It is recommended to switch off moisture analyzer's display by pressing **ON/OFF** key. On repeated pressing of the **ON/OFF** key the moisture analyzer is ready for operation and carrying out the following measurements.

9. MOISTURE ANALYZER MAIN PARAMETERS. ADJUSTING MOISTURE ANALYZER OPERATION TO AMBIENT CONDITIONS AT A WORKSTATION

- Setting filtering level – **AuE**.
- Autozero function – **Auto**.
- Access to library of drying modes – **Libr**.
- Backlight of measurement result - **bl**.
- Display brightness - **blbA**
- "Beep" sound – reaction on pressing a key – **bEEP**.

User of a moisture analyzer can adjust its operation to current ambient conditions at a workstation (by changing the value of digital filters), or according to user needs (autozero operation or display backlight) by using parameters grouped in this function.

9.1. Setting filtering level

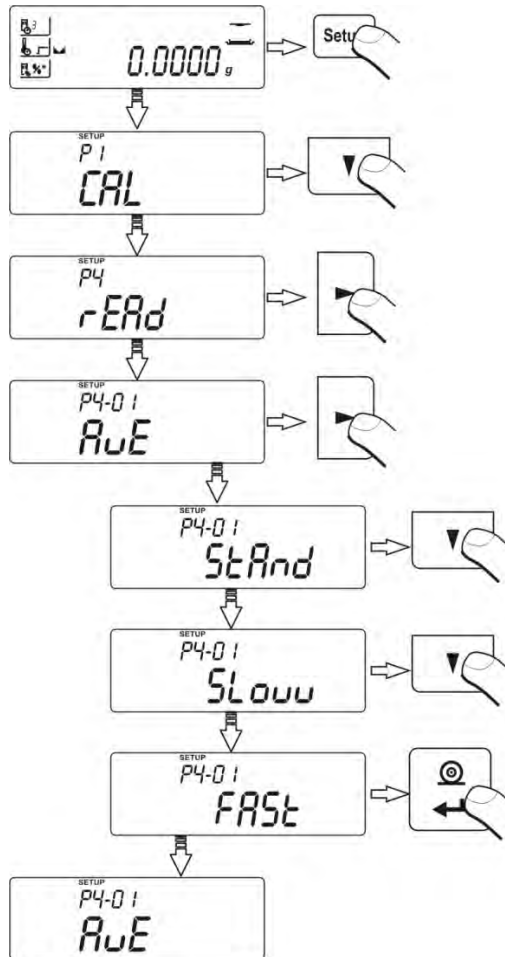

- use navigating keys to select desired filter value,

AuE = StAnd

AuE = Slouu

AuE = Fast

- (normal) – normal operation conditions,

- (slow) – harsh operation conditions – vibrations, etc.,



- (fast) – good operation conditions – no vibrations, etc.




CAUTION:

The stronger filtering setting the longer weighing time.

9.2. Autozero function

In order to ensure moisture analyzer's precise mass indication, autozero (**Auto**) software parameter has been introduced. The application of this function is automatic control and correction of zero indication. When function is enabled, it compares moisture analyzer indications at declared time interval e.g. 1 s, on conditions that weighing pan is unloaded and display indication is close to zero. If results vary less than declared AUTOZERO range e.g. one division, the moisture analyzer will zero automatically, display marker of stable measurement result  and precise zero marker **0** .

If AUTOZERO function is enabled, then each weighing process starts from precise zero point. There are, however, some cases when this function can be a disturbing factor of measuring process; for instance very slow placing of load on the weighing pan (e.g. load pouring) – in such case system of zero indication correction can also correct actual indication of loaded mass.

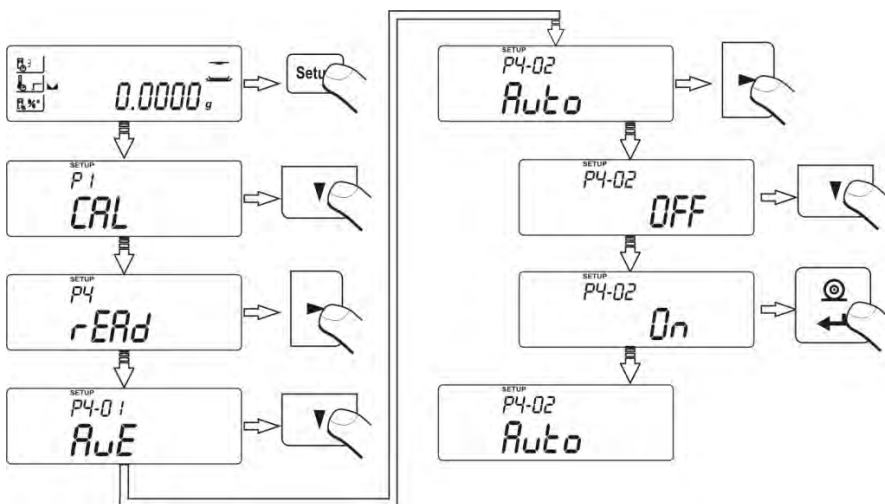


Auto = On - autozero enabled,

Auto = OFF - autozero disabled.

9.3. Access to library of drying programs


In order to use the library of drying programs set parameter <Libr> to value <YES>:

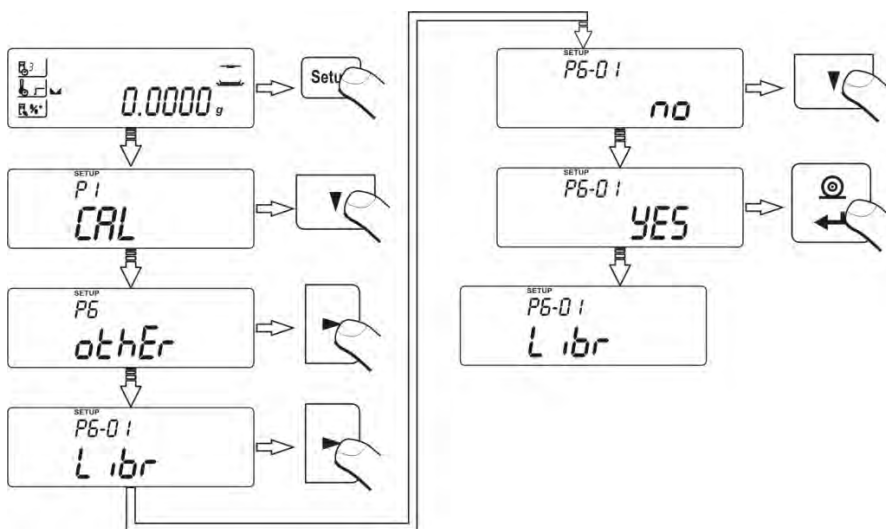

- no** - libraries of drying programs disabled,
YES - libraries of drying programs enabled.

9.4. Backlight of measurement result (display backlight)

The function enables switching on and off backlight of measurement result on the display.

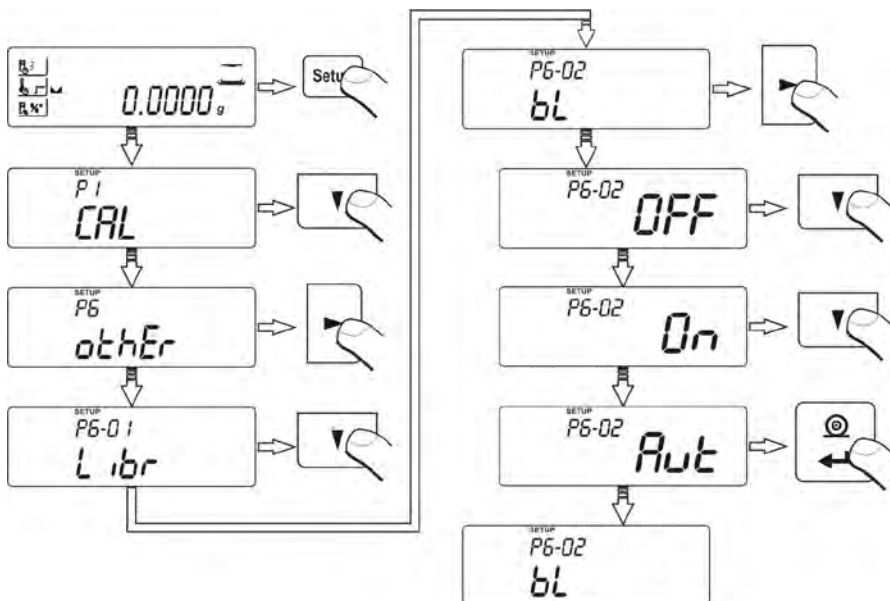


- | | |
|------------|--|
| OFF | - backlight disabled |
| On | - backlight enabled |
| Aut | - backlight disabled automatically if measured indication does not change within 10 seconds. |



CAUTION


Moisture analyzer software has implemented option of automatic backlight switch off **bl = Aut**. In case of this setting, the backlight is switched automatically off if measurement results does not change within 10 seconds. Backlight is automatically activated at the moment of weighing result change on moisture analyzer's display.

9.5. Brightness adjustment of display backlight

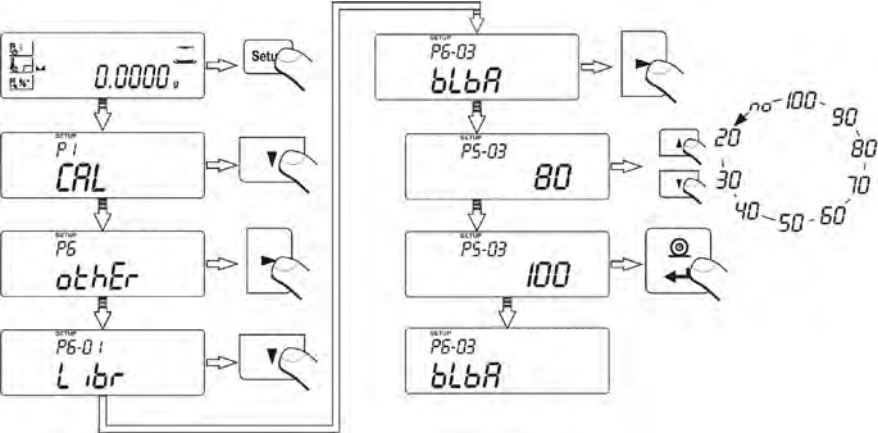

- 100 - maximum display brightness
- 20 - minimum display brightness
- no - display brightness disabled

9.6. “beep” sound – reaction on pressing a function key

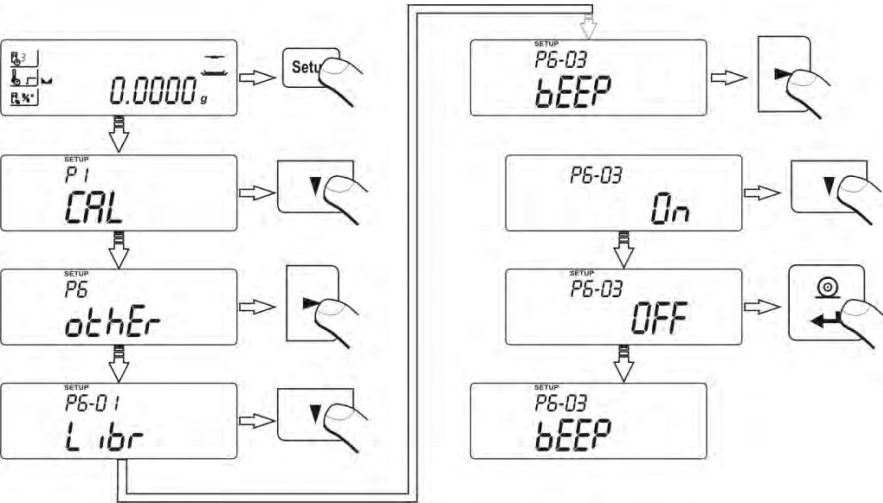

- bEEP = On - signal of pressing function key enabled,
- bEEP = OFF - signal of pressing function key disabled.

10. MOISTURE ANALYZER ADJUSTMENT

As the gravitational acceleration force has different value at various latitudes and altitudes, a moisture analyzer should be adjusted to present working conditions. This process should take place at the first installation of the instrument on site and at its every re-location – as in case of ambient temperature changes.

In order to ensure the highest weighing accuracy, it is recommended to periodically refresh moisture analyzer's accuracy by carrying out adjustment process.

Adjustment should be carried out:

- Before the beginning of measuring process,
- If long breaks between following measuring series occur.

Types of adjustment:

- adjustment with an external weight




Remember to carry out adjustment process only when there is no load on the weighing pan! In case there is load on the weighing pan, the display will indicate a command **Er1 Hi**. It is a command of unloading the pan. Adjustment process can be aborted if necessary by pressing **Esc** key!

10.1. External adjustment

External adjustment in moisture analyzer MAC series should be carried out with an external mass standard / weight class F2 or higher.

Start of external adjustment process,

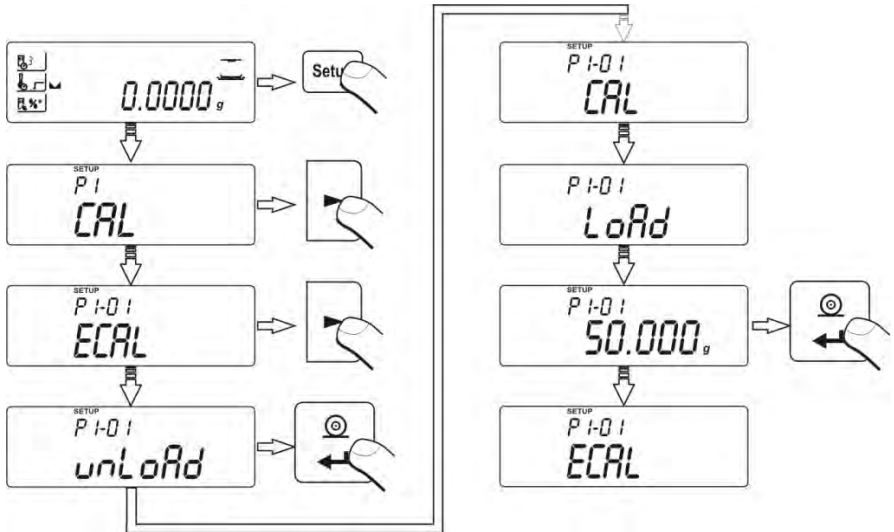

On selecting **CAL** mode, the moisture analyzer displays a command **unLoAd** – ordering unloading of the weighing pan (**the weighing pan must be empty**). When the weighing pan is empty press **Print/Enter** key. The moisture analyzer initiates adjustment procedure. In a moment the display indicates mass of a standard / weight to be loaded on the weighing pan – on loading the mass standard / weight press **Print/Enter** key. On completing adjustment process the moisture analyzer returns to submenu **P1-01 ECAL**, (if a moisture analyzer is connected to a printer or a computer, then it automatically sends a report from adjustment process to be printed – only if corresponding option has been enabled in moisture analyzer's settings).



CAUTION

- Press **ESC** key to abort adjustment process.
- If during adjustment process, weighing pan of a moisture analyzer is loaded, then moisture analyzer displays an error message **Er 1 Hi**.




Return to weighing mode

(see point 7.2 – return to weighing mode).


10.2. Adjustment test

Adjustment test is a comparison of mass of an adjustment weight with the value of last adjustment saved in moisture analyzer's memory. This process is automatic and its result is previewed on the display (if a moisture analyzer is connected to a computer or a printer through RS 232 interface, data on adjustment test is printout – only if corresponding option has been enabled in moisture analyzer's settings). Press **Print/Enter** key to return to previous display in moisture analyzer's menu structure.

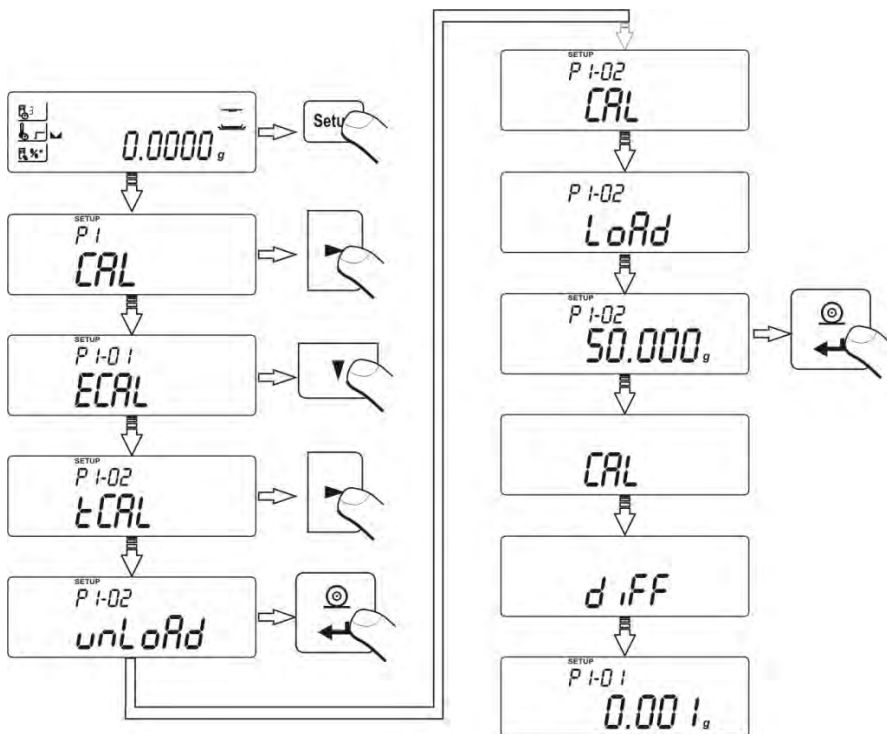


10.3. Drying chamber adjustment

Special adjustment set, which is an atypical accessory of a moisture analyzer, is used for temperature adjustment.

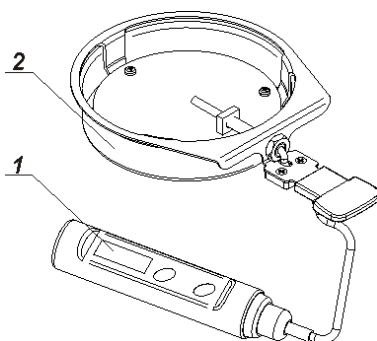

1. Thermometer
2. Thermometer holder with a holder shield


Adjustment is a process that aims at calibration of temperature sensor of a drying chamber. To proceed to temperature adjustment please insert the temperature adjustment set into the moisture analyzer. Follow instruction below:

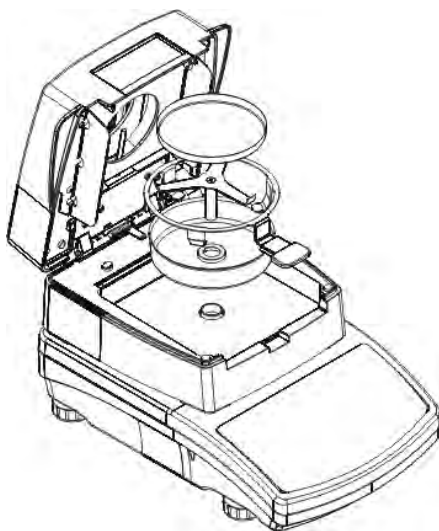

Step 1.

Displace:


- disposable drying pan
- drying pan handle
- drying pan bracket
- drying chamber cover

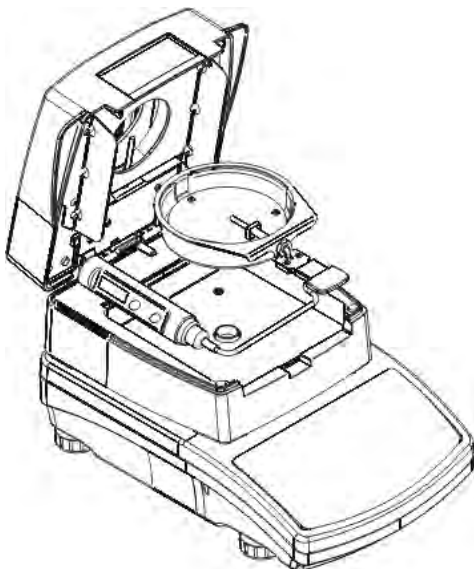

Step 2.

Insert parts of the set into the drying chamber:


- shield and thermometer

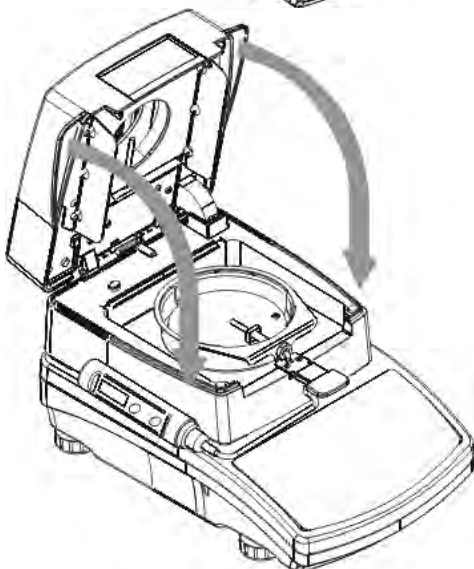

Step 3.

After set assembly close the drying chamber and start temperature adjustment.

CUTION: Use most gentle movements so as not to damage moisture analyzer's mechanism.

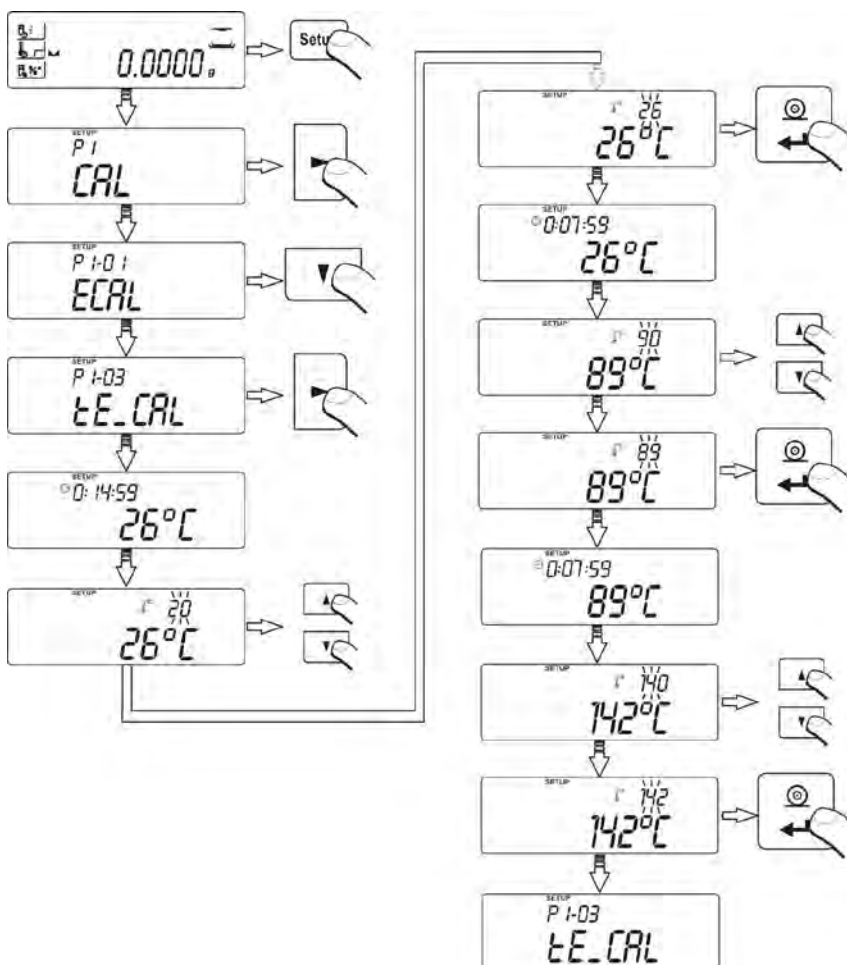

Go to menu **P1-03 tE_CAL**, adjustment process is initiated automatically. The moisture analyzer displays current temperature in the drying chamber. After 8 minutes the display indicates (pulsating) temperature value. Use navigating keys (up and down arrow) on moisture analyzer's overlay to set temperature value to be equal to the current temperature displayed on the control thermometer. Use **Print/Enter** key to start part two of temperature adjustment process. The moisture analyzer switches on the halogen lamp and heats the drying chamber to a defined temperature value. The temperature value is maintained for 8 minutes, and its value is visible on moisture analyzer's display. After 8 minutes the display indicates (pulsating) temperature value. Use navigating keys (up and down arrow) to set temperature value to be equal

to the current temperature displayed on the control thermometer – as in previous step. On entering the temperature value and accepting it by pressing **Print/Enter** key, the software starts the last part of temperature adjustment process. The moisture analyzer heats the drying chamber to another temperature value, which is maintained for 8 minutes. Current temperature of the drying chamber is visible on the display. After 8 minutes the display indicates pulsating temperature value, which should be changed to be equal to the one indicated on control thermometer (as in previous steps). On entering temperature value accept it by pressing **Print/Enter** key. Temperature adjustment process is completed, and the display indicates name of the parameter: **P1-03 tE_CAL**.

In case of moisture analyzer with maximum heating temperature 250 °C, the temperature adjustment process is the same, with only difference in higher temperature values in each part of the process.




Return to weighing mode

(see point 7.2 – return to weighing mode).

10.4. Adjustment report printout

On completing an adjustment process, the moisture analyzer enables generating a report from adjustment process. The report can be printed on a connected printer and sent to a computer and saved in a form of file for future records.

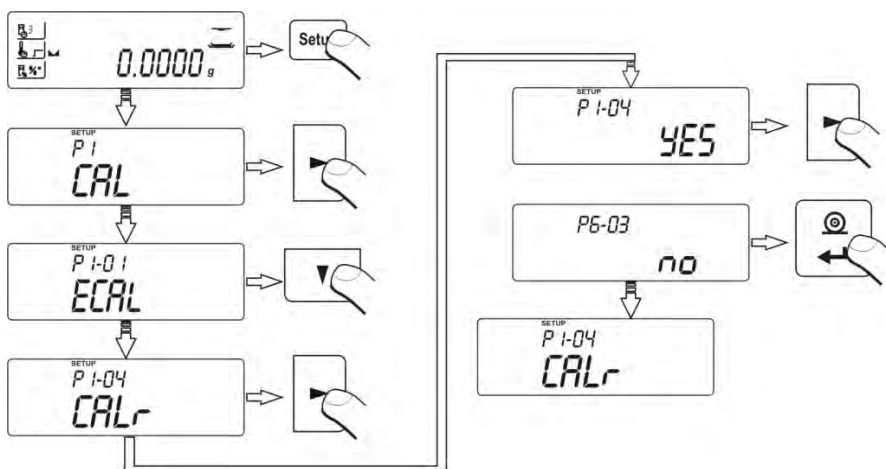

YES

- report is printed.

no

- report is not printed

Remember, that if the parameter is set to **YES**, then a report is generated and sent (printed) automatically.

Content of report from adjustment process depends on the settings of **GLP** parameters. Any option in the GLP submenu which attribute is YES is included in a report from adjustment process.

An instance of a report from adjustment process:


```
*** External calibration report ***  
  
Date       : 2007/08/08  
Time       : 12:21:57  
User Id    : WILK  
Project Id  : TEST  
Balance Id  : 100000  
  
Calibr.     : External  
Difference   : - 0.004 g  
  
Name .....
```

10.5. Drying process test

<Drying process test> parameter allows to control correctness of thermometer indications. Special adjustment set is used for test procedure of the drying chamber (thermometer and thermometer holder). The set is an atypical accessory of a moisture analyser (the same set is used for temperature adjustment of the drying chamber). See point 10.3 for assembly instruction.


To start the procedure first assembly the adjustment set into the drying chamber, next enter <CAL> menu and activate process **P1-05 tSt_Co**, follow instruction below.

After the thermometer has been assembled, close the drying chamber and proceed to the test.

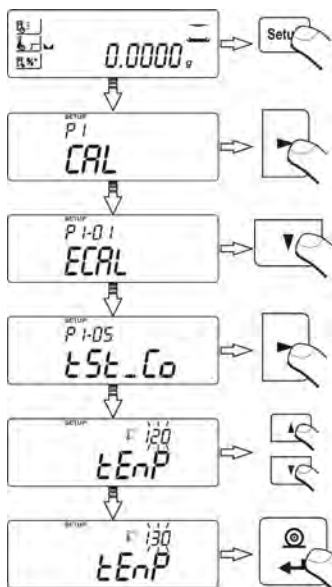


Enter **P1 CAL** menu, next start **P1-05 tSt_Co** procedure. Before the test activation set its parameters in accordance with diagram and description, to be found below.


Use navigating arrows to set specified test temperature, press ENTER to confirm.

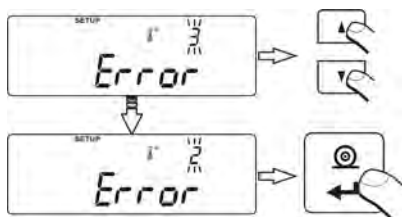


Next, enter tolerable (accepted by the user) temperature errors. Use navigating arrows to set specified error value, press ENTER to confirm.

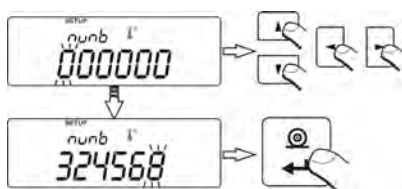

Next enter serial number of the adjustment set, which will be used for the test. Use navigating arrows to set the number, press ENTER to confirm.



Upon confirmation of the number, program will automatically start drying process until the specified temperature is reached. Time and sensor temperature information will be displayed. Temperature will remain unchanged for 8 minutes (like for temperature adjustment process).

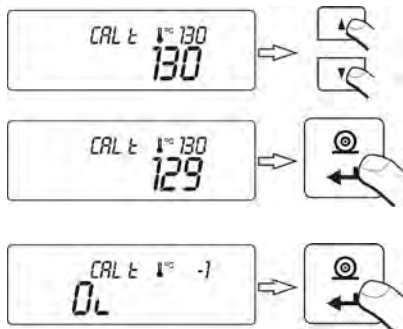

After 8 minutes the user will see a window, where temperature read from the assembled adjustment set must be entered. Use navigating arrows to set the temperature, press ENTER to confirm.

Wait to see the window with temperature error related to adjustment set temperature.

<i>Drying chamber test</i>	

Date:	2013/05/24
Time:	09:21:18
Balance Id:	349011
Calibr. Id:	324568
Set temp:	130
End temp:	130
Measured temp:	129
Acceptable error:	2
Status:	OK

The result of the test may be printed on a printer connected to the balance. To do it press PRINT button.

An instance of the report is to be found on the left.

Press Esc few times to get back to the main window.

11. DETERMINING CONTENT OF A PRINTOUT FOR GLP PROCEDURES


Group of parameters P2 GLP enables declaring variables that are present on an adjustment printout and printout activated after a measurement.

P2 GLP

P2.1	USr		
P2.2	PrJ		
P2.3	Ptin		YES
P2.4	PdAt		YES
P2.5	PUSr		YES
P2.6	PPrJ		YES
P2.7	PId		YES
P2.8	PFr		YES

- **P2-01 USr**

The parameter enables determining name of an operator who works with a moisture analyzer. User name contains maximally 6 alphanumeric characters. User name is inserted using moisture analyzer's keyboard and navigating arrows **Up**, **Down**, **Left**, **Right**.

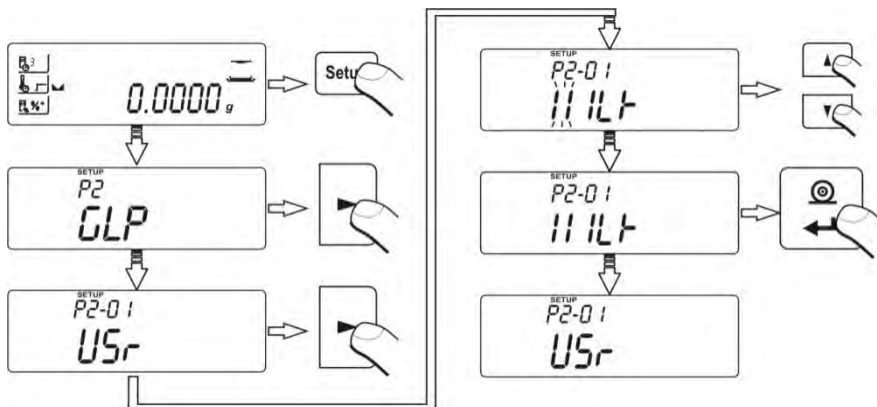

Accessible characters and their equivalents displayed by the moisture analyzer:

-	0	1	2	3	4	5	6	7	8	9		
—	0	1	2	3	4	5	6	7	8	9		
A	b	c	d	E	F	G	H	I	J	K	L	M
A	B	C	D	E	F	G	H	I	J	K	L	M
n	0	P	q	r	S	t	U	V	W	X	Y	Z
N	O	P	Q	R	S	T	U	V	W	X	Y	Z
d	b	c	d	e	F	g	h	i	J	k	l	M
a	b	c	d	e	f	g	h	i	j	k	l	M
n	o	P	q	r	S	t	u	v	w	x	y	z
n	o	P	q	r	s	t	u	v	w	x	y	z

An instance of a user name inserted to a moisture analyzer using capital letters takes below form:



WILK

An instance of a user name inserted to a moisture analyzer using small letters takes below form:



- **P2-02 Prj**

The parameter enables determining name of a project (e.g. related to a specific type of carried out test).

An instance of project name inserted to a moisture analyzer using capital letters takes below form:



An instance of project name inserted to a moisture analyzer using small letters takes below form:



- **P2-03 Ptin**

Option determining presence of measurement time on a printout.

- **P2-04 PdAt**

Option determining presence of measurement date on a printout.

- **P2-05 PUSr**


Option determining presence of user name on a printout.

- **P2-06 PPrj**

Option determining presence of project name on a printout.

- **P2-7 PlId**


12.2. Setting date

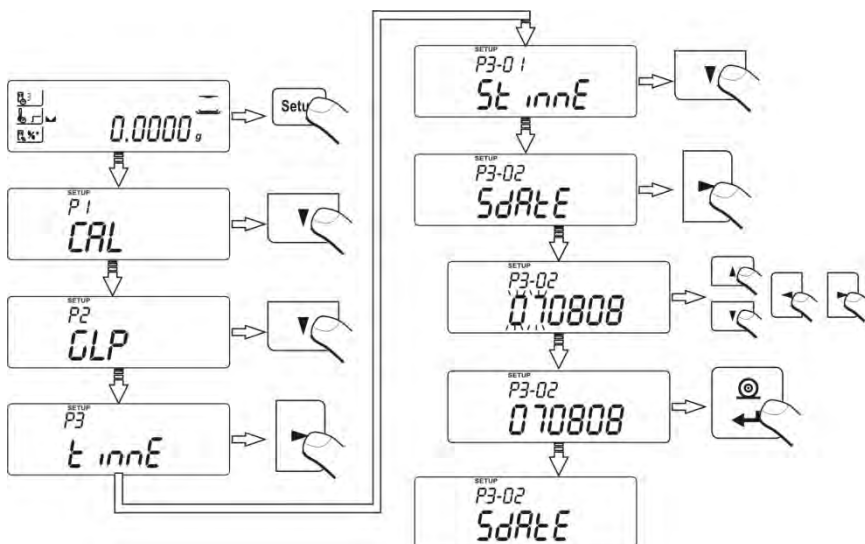

This parameter enables setting date in a moisture analyzer. In order to change date settings use navigating keys **Up**, **Down**, **Left**, **Right**.

13. RS 232 FUNCTIONS

13.1. Baud rate setting

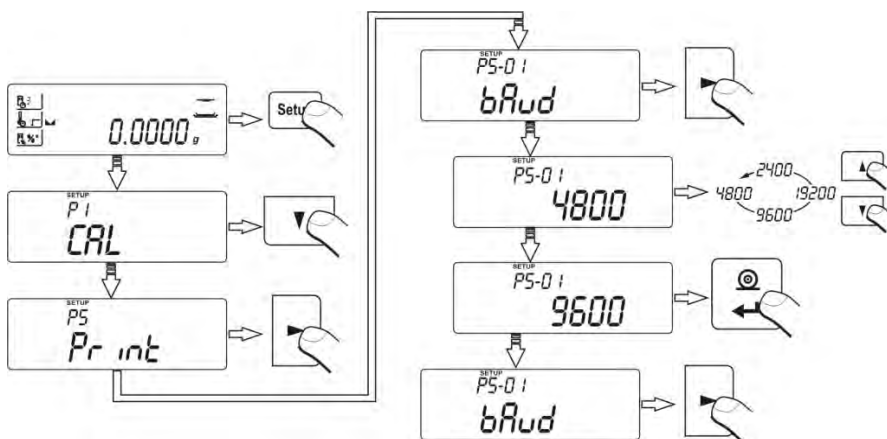

Select one of available baud rates:


- 2400 bit/s
- 4800 bit/s

- 9600 bit/s
- 19200 bit/s.



Return to weighing mode
(see point 7.2 – return to weighing mode).

13.2. Determining data type sent via RS 232 output

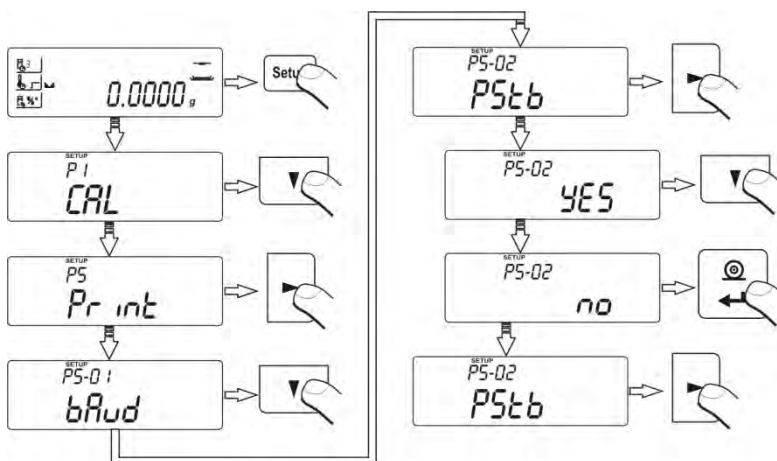


YES
no

- sending stable measurement result,
- sending stable or temporary (unstable) measurement result.




Return to weighing mode
(see point 7.2 – return to weighing mode).

13.3. Printout interval

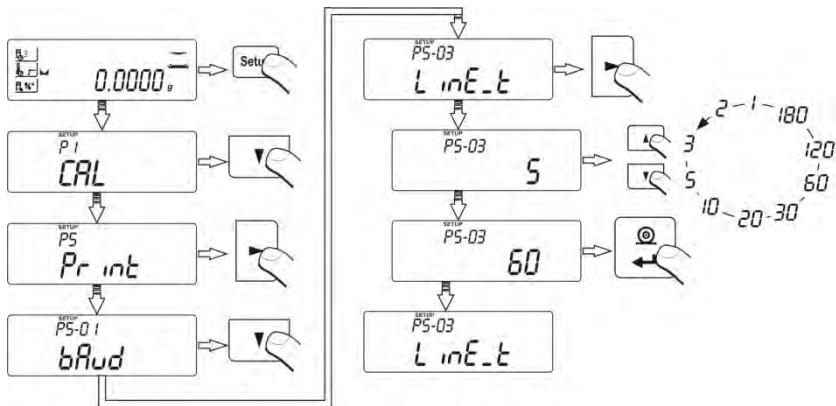

Printout interval determines how often data on drying process is sent through RS 232 port. Available settings: 1, 2, 3, 5, 10, 20, 30, 60, 120, 180 seconds (setting <----> results in printing only a header and a footer – respectively, drying process start and drying process end, halfway results are not printed – line).

13.4. Determining range of data sent during drying process

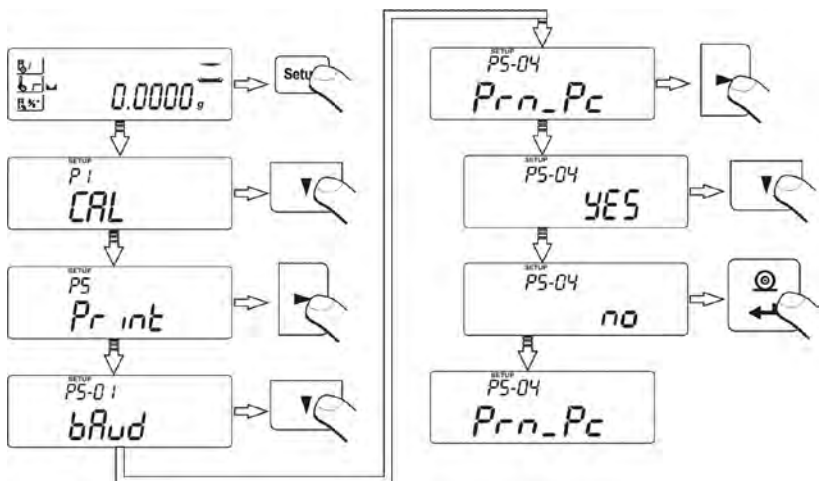

- YES** - data limited to drying process result only (printout of a single line).
- no** - printout of complete report from drying process: header, line, footer.



Return to weighing mode

(see point 8.2 – return to weighing mode).

14. DRYING PROCESS WITH USE OF SHORTENED MENU


Menu of drying mode enables setting the following parameters:

- means of drying process auto switch off mode,
- drying mode for carrying out the drying process,
- type of displayed measurement result.


In order to start drying process with use of shortened menu, disable access to libraries of drying programs – go to menu – **P6-01 Libr.**

In order to change parameter settings, enter the drying menu by pressing **Test menu** key. Marker of submenu group **drying process auto switch off mode** starts flashing. Then, using **Right** navigating key enable menu of changing settings of this parameter group. Use navigating keys **Up** and **Down** to set one of available options and accept changes (by double pressing of **Print/Enter** key) or continue parameter settings (single pressing of **Print/Enter** key).

14.1. Setting means of auto switch off mode

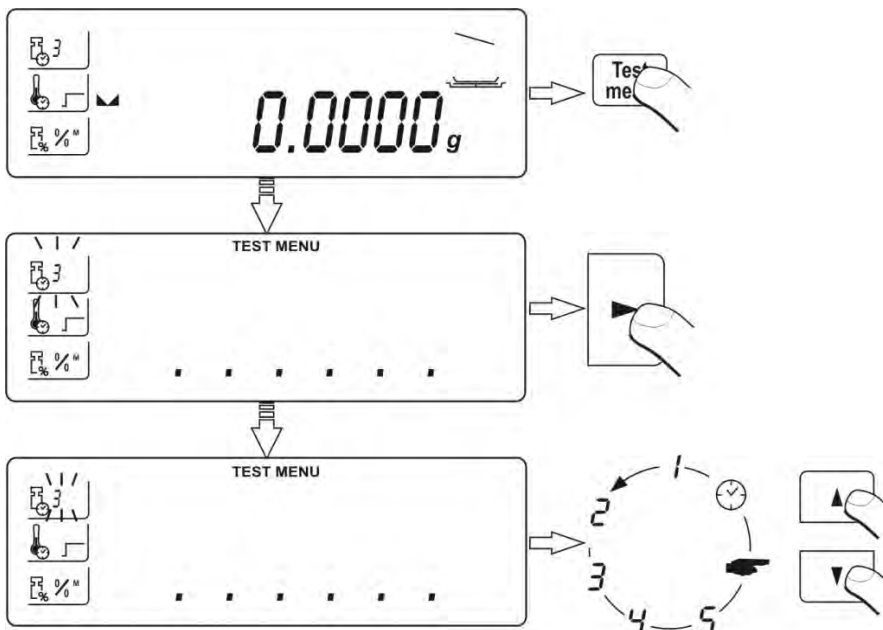


Parameter **switch off mode** can take the following values:

- 1 – automatic finish (mass change 1mg / in 10s time)
- 2 – automatic finish (mass change 1mg / in 25s time)
- 3 – automatic finish (mass change 1mg / in 60s time)
- 4 – automatic finish (mass change 1mg / in 90s time)
- 5 – automatic finish (mass change 1mg / in 120s time)
-  - manual finish (on pressing **Start/Stop** key)

Maximal time interval of the drying process cannot be longer than 9 hours 59 minutes. After this time the process will be automatically switched off.




- time defined (max time setting 9 hours 59 minutes):

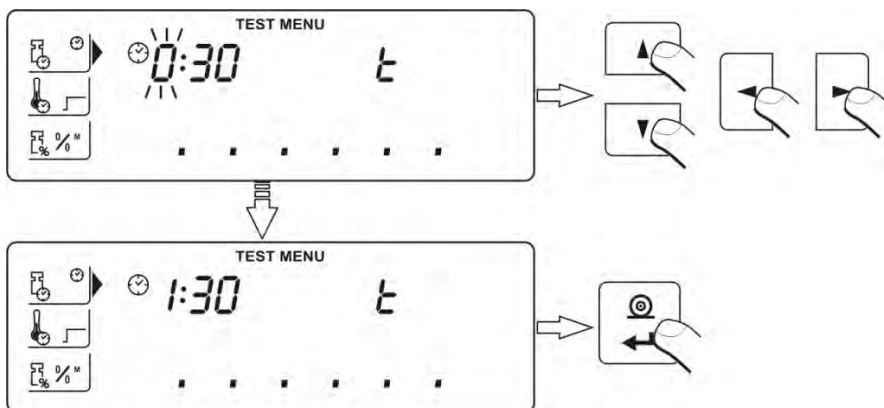

In order to accept carried out changes, press **Print/Enter** key for three (3) times.

14.2. Active drying mode

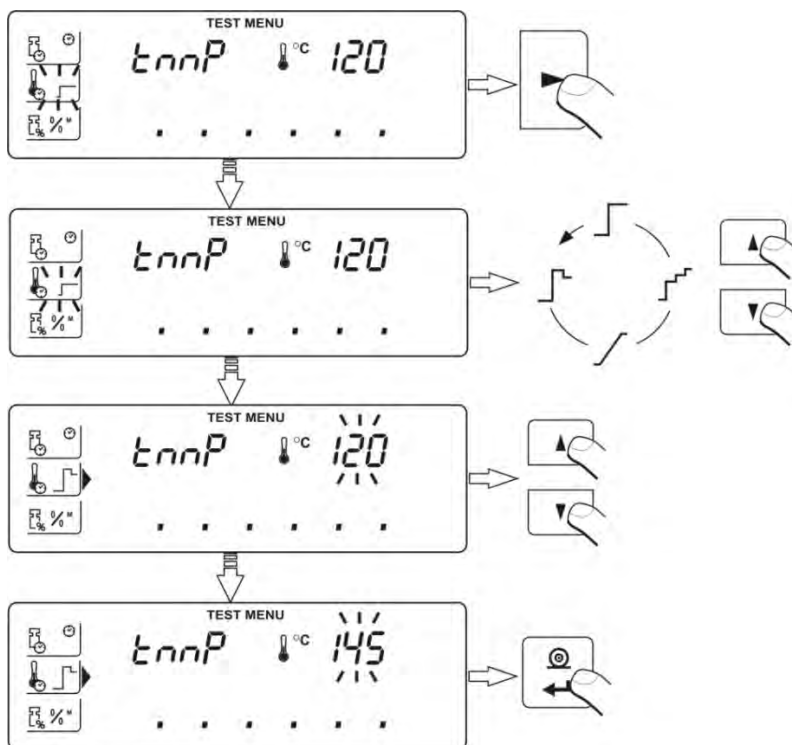

In order to accept carried out changes, press **Print/Enter** key for three (3) times.

Parameter **active drying mode** can take the following values:

- Drying mode **STANDARD**




In standard mode, user should set drying temperature **tmP** in which a sample should be tested,

- Drying mode **QUICK**



In quick mode, user should set drying temperature **tmP** in which a sample should be tested,



Specific feature of this drying mode is fast increase of drying temperature in short period of time. Drying temperature for the time of 180 seconds is exceeding the pre-set value by 30 %, after which is drops to temperature value set in the parameters of the drying mode.

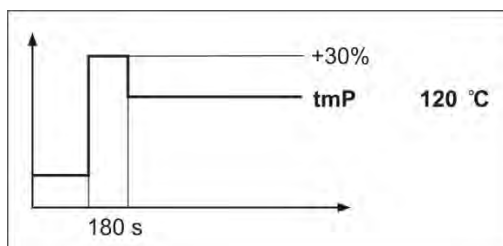

- Drying mode **MILD**




In mild mode, user should set drying temperature **tmP** in which a sample should be tested, and time **t1** in which a moisture analyzer should reach pre-set temperature value.

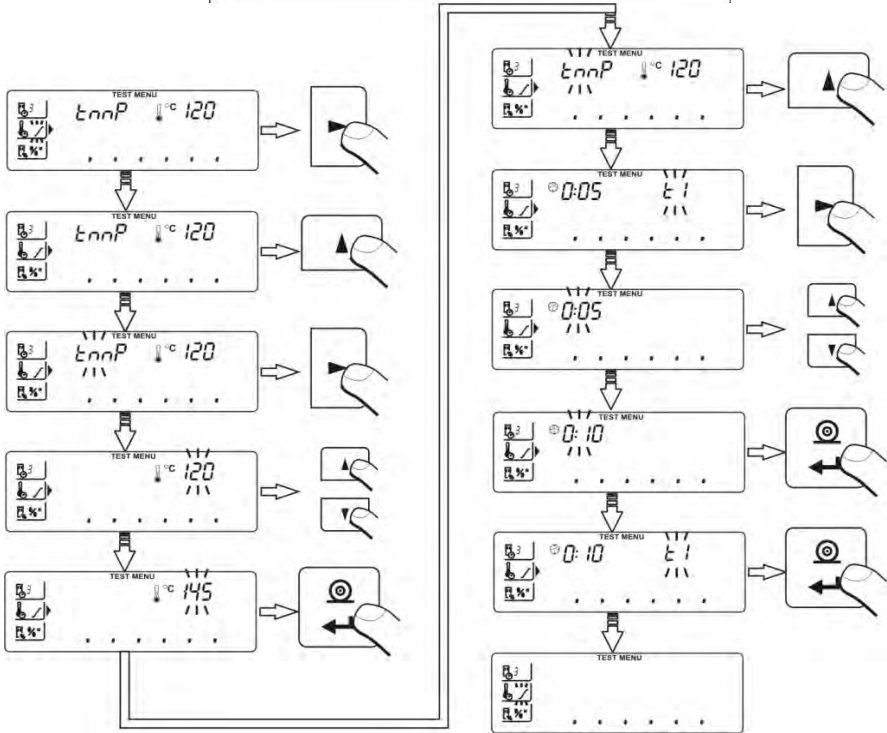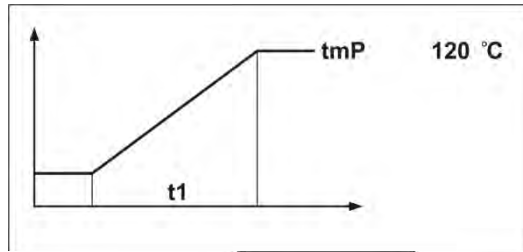

- Drying mode **STEP**



In step mode, user should set drying temperature **tmP** in which a sample should be tested, temperature values **tmP1** and **tmP2** and time values **t1** and **t2** between reaching the temperature values in each of the steps.

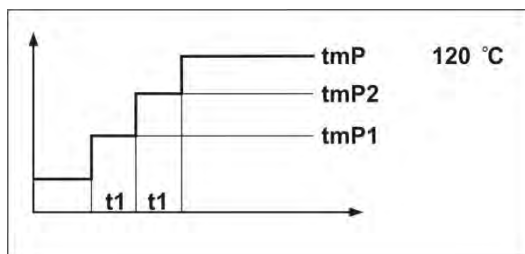


CAUTION:

For drying mode **Quick** the user must set the drying temperature and time interval of heating in temperature 30% higher than the specified temperature. Time interval of heating starts at the moment when the temperature has been reached.

For drying mode **Step** the user must set threshold temperature values „1” and „2”, drying temperature and time intervals of heating for particular intermediate temperatures (1 and 2). Time interval of heating for a given step starts at the moment when the temperature has been reached for the given step.

14.3. Type of displayed measurement result

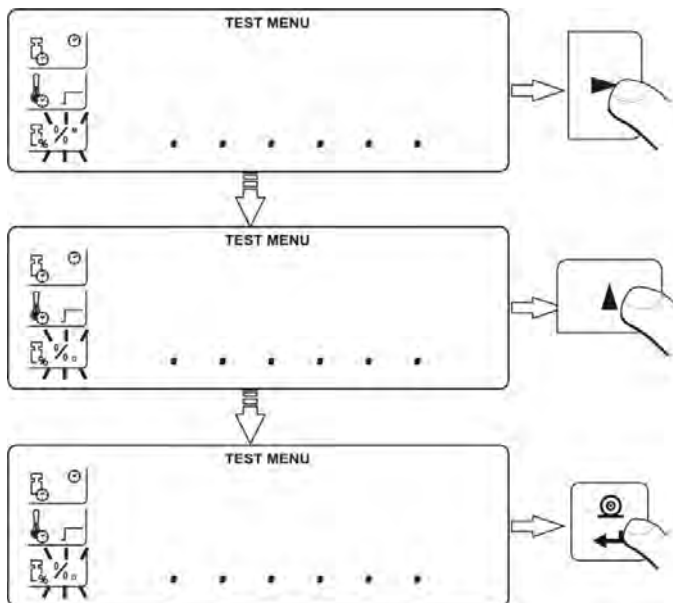

In order to accept carried out changes, press **Print/Enter** key for two times.

- Percent loss of mass

$\frac{0}{0}^M$

Displays mass change recorded during drying process, and expressed in percent,

- Part of dry mass obtained in drying process, and expressed in percent

$\frac{0}{0}^D$

Measurement result is part of mass that is remaining on the drying pan after humidity content evaporation,

- Humid / dry ratio obtained as a result of drying process, and expressed in percent.

$\frac{0}{0}^R$

Measurement result is part of mass that evaporated from the dried sample in drying process,

- Mass change


g

Measurement result is mass change recorded by the moisture analyzer in the drying process.

15. DRYING PROCESS WITH USE OF DRYING PROGRAM LIBRARY

In order to start drying process with use of drying program library, the user has to enable access to the libraries in moisture analyzer's menu: parameter – **P6-01 Libr** has to be attributed **<YES>** (see point 9.3. of this user manual). The moisture analyzer MAC series can comprise up to 20 drying procedures / programs, which are optionally configured, saved and used by selecting one of them.

Should one of drying procedures / programs be used, follow below guidelines:

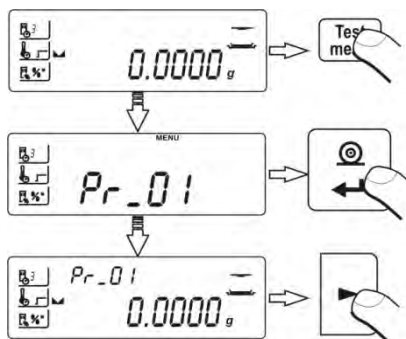

In order to exit the option of using drying program libraries, disable access to libraries in moisture analyzer's menu (**see point 9.3. of this user manual**).




Changing settings of any drying program (auto switch off mode, drying mode, drying temperature, data to be displayed and printed) in the library, requires selecting one of drying programs, and then acting as specified in **point 14: DRYING PROCESS WITH USE OF SHORTENED MENU**.

Additionally, each drying procedure stored in the library allows for using an option of sample mass control. When enabling the option, a moisture analyzer software informs the user whether the mass to be tested is within set thresholds, regarding the mass and tolerance values, on condition that the parameters were determined for the sample. The sample mass control is visualized by displaying pictograms LO, OK or HI on moisture analyzer display. The option is implemented for information purpose only and facilitates a user in preparing the same or very similar sample to be tested, thus increasing repeatability of measurements. If the pre-determined mass control criteria are not met (i.e. pictograms LO or HI are displayed), the moisture analyzer still starts the drying process. Settings of mass control option are provided below.


15.1. Sample mass control

Sample mass control option is active only in case of enabled access to library of drying programs – P6-01 Libr (parameter set to YES).


The mass control value and tolerance value are set in the following way:

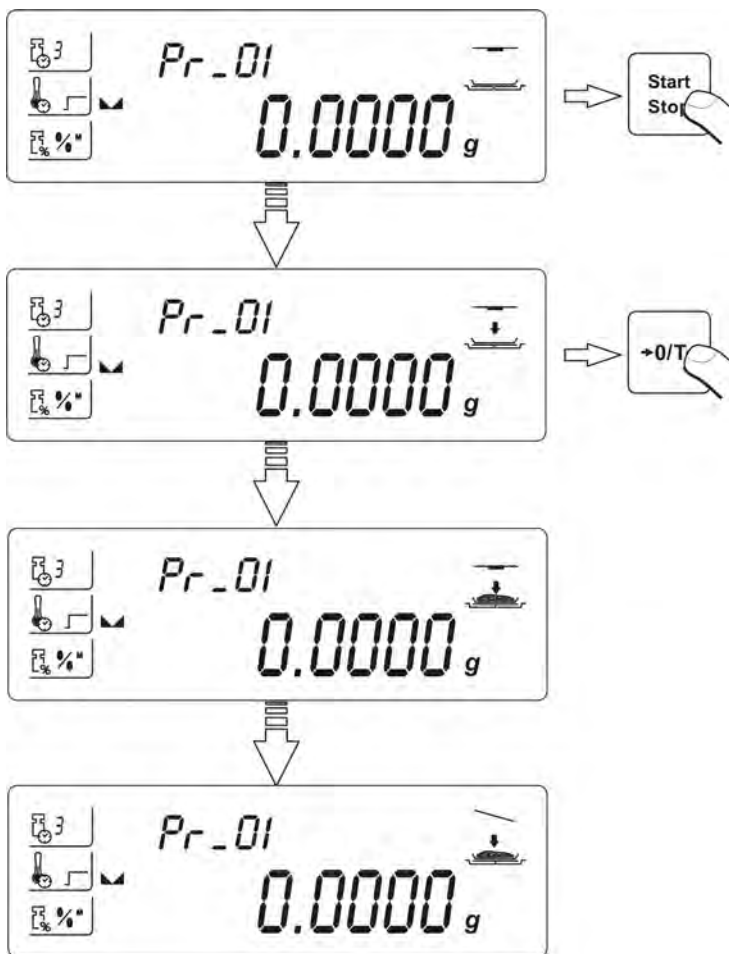


Start drying process by pressing **Start/Stop** key, and on emptying moisture analyzer's drying pan, pressing **TARE** key. Open the drying chamber's lid, place test sample on the drying pan, and close the drying chamber's lid.

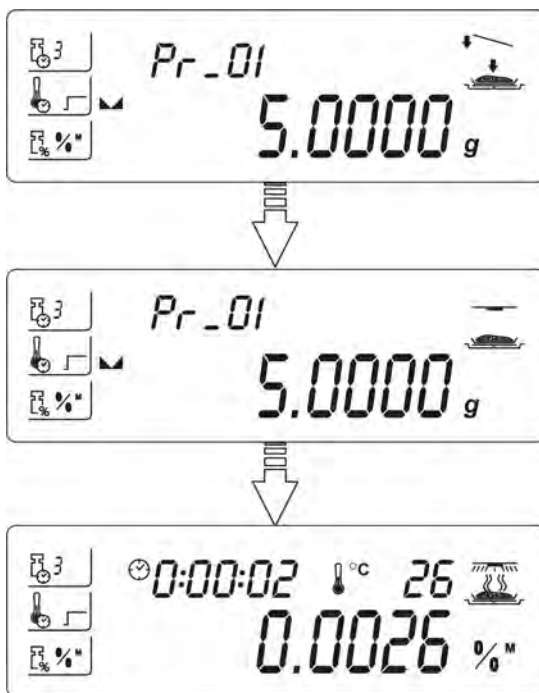

Changing of displayed data during drying process is carried out by pressing **Display** key.

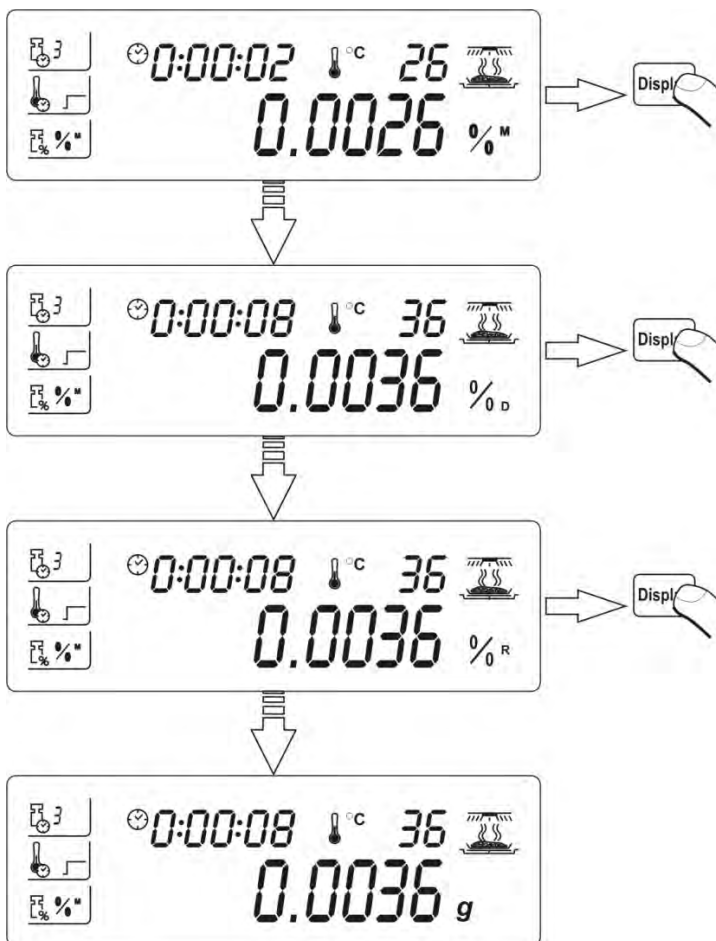

In order to abort drying process, press **Start/Stop** key and accept switch off mode of drying process by pressing **Print/Enter** key. An exception from the above procedure is means of aborting the drying process in manual mode – on pressing **Start/Stop** key the moisture analyzer aborts drying process with no need to confirm the action by pressing **Print/Enter** key.

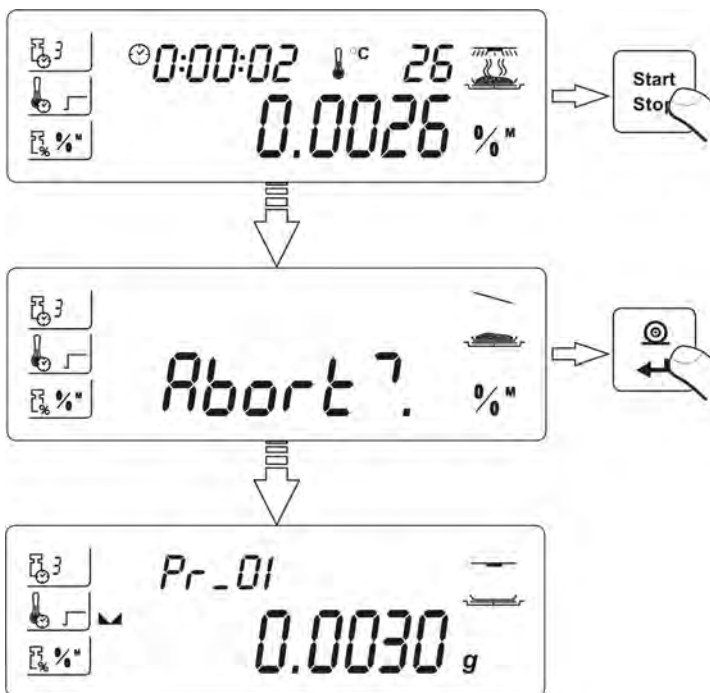

17. SET OF COMPUTER – MOISTURE ANALYZER COMMANDS

Function INTERFACE RESET

Command **R CR LF** (zeroing of currently carried out commands, i.e. “tare” which waits for stable result).

Function SEND ALL IMPLEMENTED COMMANDS FROM THE INSTRUMENT

Command **PC CR LF** (sends information on all implemented commands in the program from the instrument)

Function SEND STABLE RESULT IN BASIC UNIT

Command **S CR LF** (sends result in basic unit from the instrument on stable mass readout)

Function IMMEDIATELY SEND THE RESULT IN BASIC UNIT

Command **SI CR LF** (sends result in basic unit from the instrument)

Function SEND THE RESULT IN CURRENT UNIT

Command **SU CR LF** (sends the result in current used result on stable mass readout)

Function Command	IMMEDIATELY SEND THE RESULT IN CURRENT UNIT SUI CR LF (sends the result in current used unit from the instrument)
Function Command	ZERO THE INDICATION Z CR LF (zeroes the indication on stable readout)
Function Command	TARE WHEN STABLE T CR LF (TARE the indication on stable readout)
Function Command	SWITCH OFF CONTINUOUS TRANSMISSION IN BASIC UNIT C0 CR LF (stops continuous transmission in basic unit)
Function Command	SWITCH ON CONTINUOUS TRANSMISSION IN BASIC UNIT C1 CR LF (starts continuous transmission in basic unit)
Function Command	GIVE SERIAL NUMBER OF THE INSTRUMENT NB CR LF (sends factory number)
Function Command	GIVE WEIGHING RANGE FS CR LF (send instrument's value of max capacity in basic unit)
Function Command	GIVE SOFTWARE VERSION RV CR LF (sends name and version of the instrument's software)
Function Command	SEND SETUP PS CR LF (sends all instrument's setup – printout of the parameters)

Caution!



*Sending a command to the instrument which is not in the above list or has an error, and it is finished with CR LF, causes instrument's response in format **E S CR LF**. Spaces provided in the command formats should be omitted, as they are given for proper legibility of the commands.*

18. ERROR MESSAGES

If moisture balance software detects an error a proper error message appears on the graphic display. The error message contains number of error which informs about its source.

Error message	Error description
Er1 Hi	Start mass exceeds permissible range (it refers to start and adjustment – start mass)
Er2 nu	Low limit of converter range exceeded
Er3 Fu	High limit of converter range exceeded
Er4 ro	Value of mass or temperature exceeds permissible range (it refers to mass or temperature adjustment – final mass or temperature)
Er5 Ad	A/D converter error
Er6 to	Operation time exceeded (tarring or printing caused by lack of stability status in set time)
Er7 ou	Inserted value is out of range (reg. setting reference mass, date, etc.)

19. PRINCIPLES OF USE

For measurement temperatures ranging from 161°C to 250°C time interval for temperature maintenance is estimated proportionally as follows, 60 min for 161°C – 20 min for 250°C.

For drying process in temperature 250°C, Max temp is maintained for 20 min, next the program automatically lowers the temperature to 161°C, without aborting the drying process.

Time interval for lowering the temperature to 160°C is 20 min.

For drying mode **Quick** overdriving Max drying temperature is 30% but no more than Max default temperature.

For drying mode **Step** time interval for temperature maintenance is limited to 20 minutes for particular steps.

PRIOR VERSION OF MOISTURE ANALYZER

Parameter <P6-06Preuer> must be set to value <YES>.

Parameter allowing the moisture analyser to be operated by means of a prior version of the software (valid since June 2013). Upon setting parameter **<P6-06Preuer>** to value **<YES>** the moisture analyzer operates like its prior version (produced before June 2013) in terms of drying temperatures and drying process control (when operating in similar temperature conditions).

This allows using drying process settings the same like for previous moisture analyzers of this series. Thus the user does not have to set the drying parameters for a newly purchased product, he may work with already set ones.

*User manual no.:
IMMU-12-03-04-14-ENG*

MANUFACTURER
OF ELECTRONIC WEIGHING INSTRUMENTS



RADWAG BALANCES AND SCALES
POLAND, 26 – 600 Radom, Bracka 28

Phone. +48 48 38 48 800, fax. + 48 48 385 00 10

export@radwag.com

www.radwag.com

